

# INTERNATIONAL GEMMOLOGICAL INSTITUTE

SCIENTIFIC LABORATORY FOR IDENTIFICATION AND GRADING OF DIAMONDS AND COLORED STONES

Registered offices and Laboratories p.v.b.a.  
SCHUPSTRAAT 1/7  
ANTWERP - BELGIUM  
☎ 03/231 68 45 (6 L.)  
TELEX: 35228 I.G.I.



## DIAMOND CERTIFICATE


LABORATORY REPORT (ORIGINAL)		DATE: ANTWERP,
TO WHOM IT MAY CONCERN	Certificate Number: F1154269	6th July 1987

DESCRIPTION: NATURAL DIAMOND  
SHAPE AND CUT: ROUND BRILLIANT  
WEIGHT: 0.25 Carat  
MEASUREMENTS: APPROX. 4.12 - 4.18 x 2.37 mm.

PROPORTIONS and FINISH

Total depth Percentage 57.30 %  
Table Diameter Percentage 68 %  
Crown height percentage 10 %  
Pavillon depth percentage 43 %  
CULET SIZE: MEDIUM  
GIRDLE THICKNESS: MEDIUM (POLISHED)  
FINISH: Polish / Sym&Prop VERY GOOD / GOOD  
CLARITY GRADE (10 x): INTERNALLY FLAWLESS  
COLOR GRADE: G. (1)  
FLUORESCENCE: NONE

The symbols do not usually reflect the size of the characteristics.  
Red symbols indicate internal characteristics,  
green indicate external.

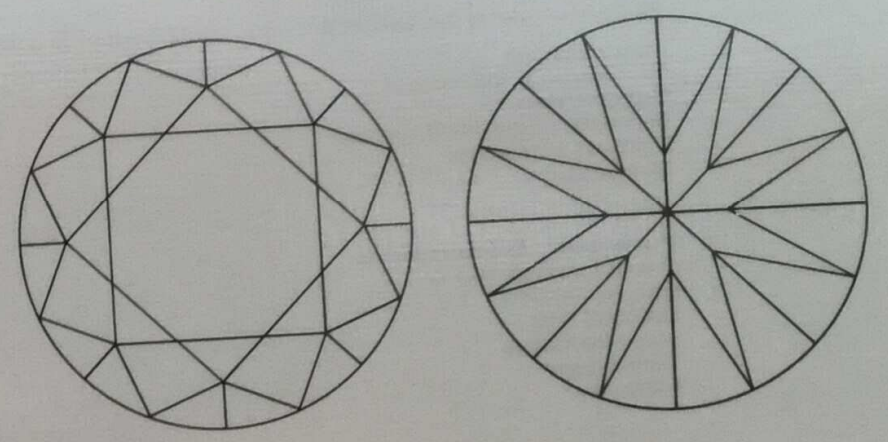

COMMENTS:  
(insignificant external details, visible only under high magnification, are not mentioned)

Control Department

*[Signature]*  
LABORATORY DIRECTOR, GEMMOLOGIST

SPACE FOR DOUBLE-CHECK, CLARITY- AND COLOR GRADE

CLARITY GRADE:	Flawless, internally FL	vvs 1	vvs 2	vs 1	vs 2	si 1	si 2	p 1	p 2	p 3								
COLOR GRADE:	0+	0	1+	1	2	3	4	5	6	7	8	9	10	11	12	13	20	FANCY COLOR
	D	E	F	G	H	I	J	K	L	M	N	O	P	Q	R			

PROPORTIONS - MARGIN ± 1%  
MEASUREMENTS - MARGIN ± 0.02 mm.  
This report is subject to the terms and conditions set forth on the reverse.

# INTERNATIONAL GEMMOLOGICAL INSTITUTE

SCIENTIFIC LABORATORY FOR IDENTIFICATION AND GRADING  
OF DIAMONDS AND COLORED STONES

Registered offices and  
Laboratories p.v.b.a.  
SCHUPSTRAAT 1/7  
ANTWERP - BELGIUM  
☎ 03/231 68 45 (6 L.)  
TELEX: 35228 I.G.I.



## DIAMOND CERTIFICATE

### LABORATORY REPORT (ORIGINAL)

TO WHOM IT MAY CONCERN	Certificate Number :	DATE : ANTWERP,
	F1I54271	6th July 1987

DESCRIPTION : NATURAL DIAMOND

SHAPE AND CUT : ROUND BRILLIANT

WEIGHT : 0.25 Carat

MEASUREMENTS \* : APPROX. 4.14 - 4.21 x 2.40 mm.

PROPORTIONS and FINISH

Total depth Percentage 57.50 %

Table Diameter Percentage 66 %

Crown height percentage 10 %

Pavillon depth percentage 43 %

CULET SIZE : MEDIUM

GIRDLE THICKNESS : MEDIUM (POLISHED)


FINISH : Polish / Sym&Prop VERY GOOD / GOOD

CLARITY GRADE (10 x) : INTERNALLY FLAWLESS

COLOR GRADE : G. (1)

FLUORESCENCE : NONE

The symbols do not usually reflect the size of the characteristics.  
Red symbols indicate internal characteristics,  
green indicate external.

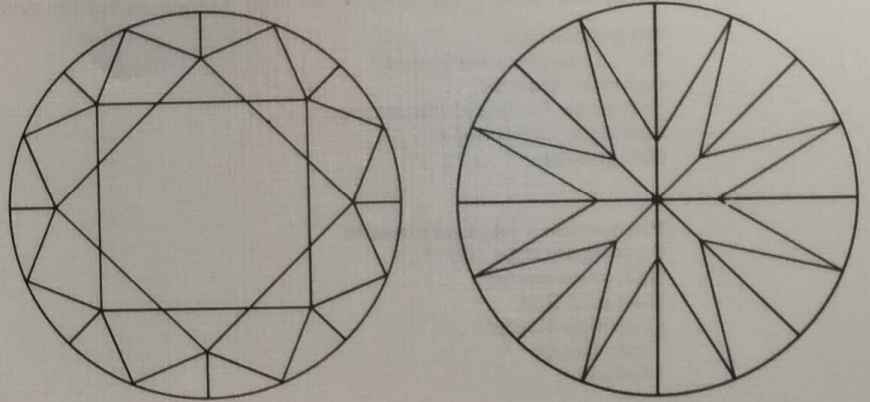

COMMENTS :

(insignificant external details, visible only under high magnification, are not mentioned)

Control Department

LABORATORY DIRECTOR, GEMMOLOGIST

SPACE FOR DOUBLE-CHECK, CLARITY- AND COLOR GRADE

CLARITY GRADE:	Flawless, internally	Fl	vvs 1	vvs 2	vs 1	vs 2	si 1	si 2	p 1	p 2	p 3							
COLOR GRADE:	0+	0	1+	1	2	3	4	5	6	7	8	9	10	11	12	13	20	FANCY COLOR
	D	E	F	G	H	I	J	K	L	M	N	O	P	Q	R			

PROPORTIONS - MARGIN : ± 1%.

\* MEASUREMENTS - MARGIN : ± 0.03 mm.

This report is subject to the terms and conditions set forth on the reverse.

# INTERNATIONAL GEMMOLOGICAL INSTITUTE

SCIENTIFIC LABORATORY FOR IDENTIFICATION AND GRADING  
OF DIAMONDS AND COLORED STONES

Registered offices and  
Laboratories p.v.b.a.  
SCHUPSTRAAT 1/7  
ANTWERP - BELGIUM  
☎ 03/231 68 45 (6 L.)  
TELEX: 35228 I.G.I.



## DIAMOND CERTIFICATE

### LABORATORY REPORT (ORIGINAL)


TO WHOM IT MAY CONCERN	Certificate Number :	DATE : ANTWERP,
	F1I54278	6th July 1987

DESCRIPTION : NATURAL DIAMOND  
SHAPE AND CUT : ROUND BRILLIANT  
WEIGHT : 0.29 Carat  
MEASUREMENTS : APPROX. 4.36 - 4.40 x 2.48 mm.

The symbols do not usually reflect the size of the characteristics.  
Red symbols indicate internal characteristics,  
green indicate external.

#### PROPORTIONS and FINISH

Total depth Percentage 56.80 %  
Table Diameter Percentage 66 %  
Crown height percentage 11 %  
Pavillon depth percentage 43 %  
CULET SIZE : MEDIUM

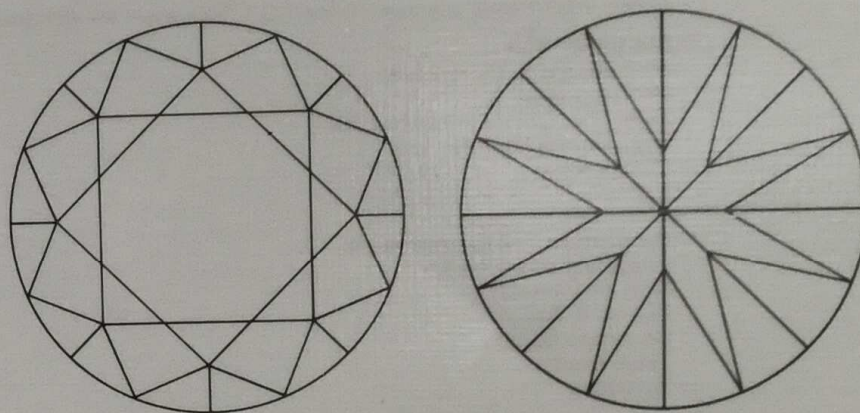

#### COMMENTS :

(insignificant external details, visible only under high magnification, are not mentioned)

GIRDLE THICKNESS : MEDIUM (POLISHED)

FINISH : Polish / Sym&Prop VERY GOOD / VERY GOOD

CLARITY GRADE (10 x) : INTERNALLY FLAWLESS

COLOR GRADE : G. (1)

FLUORESCENCE : NONE

Control Department

LABORATORY DIRECTOR, GEMMOLOGIST

#### SPACE FOR DOUBLE-CHECK, CLARITY- AND COLOR GRADE

CLARITY GRADE :	Flawless, internally FL	vvs 1	vvs 2	vs 1	vs 2	si 1	si 2	p 1	p 2	p 3														
COLOR GRADE :	0+	0	1+	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	FANCY COLOR

PROPORTIONS - MARGIN : ± 1%

\* MEASUREMENTS - MARGIN : ± 0.03 mm.

This report is subject to the terms and conditions set forth on the reverse.

# INTERNATIONAL GEMMOLOGICAL INSTITUTE

SCIENTIFIC LABORATORY FOR IDENTIFICATION AND GRADING  
OF DIAMONDS AND COLORED STONES

Registered offices and  
Laboratories p.v.b.a.  
SCHUPSTRAAT 1/7  
ANTWERP - BELGIUM  
☎ 03/231 68 45 (6 L.)  
TELEX: 35228 I.G.I.



## DIAMOND CERTIFICATE

### LABORATORY REPORT (ORIGINAL)


TO WHOM IT MAY CONCERN	Certificate Number : <b>F1I54314</b>	DATE : ANTWERP, <b>7th July 1987</b>
------------------------	---	---

DESCRIPTION : NATURAL DIAMOND  
SHAPE AND CUT : ROUND BRILLIANT  
WEIGHT : 0.29 Carat  
MEASUREMENTS : APPROX. 4.48 - 4.54 x 2.49 mm.

The symbols do not usually reflect the size of the characteristics.  
Red symbols indicate internal characteristics,  
green indicate external.

#### PROPORTIONS and FINISH

Total depth Percentage 55.20 %  
Table Diameter Percentage 64 %  
Crown height percentage 10 %  
Pavillon depth percentage 43 %  
CULET SIZE : POINTED

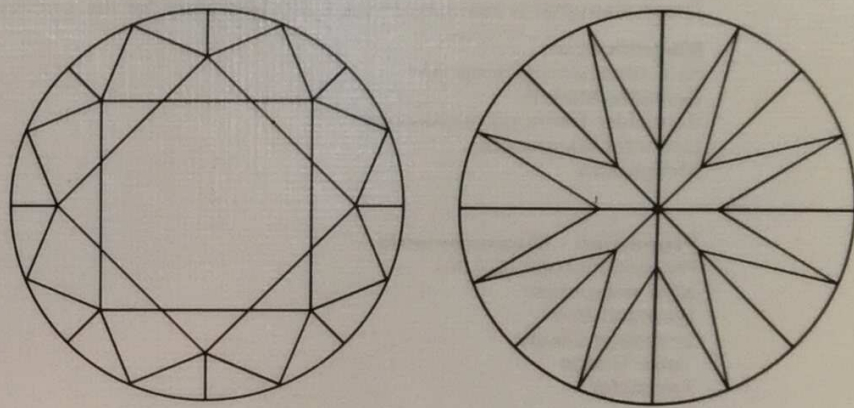

GIRDLE THICKNESS : MEDIUM

FINISH : Polish / Sym&Prop VERY GOOD / GOOD

#### COMMENTS :

(insignificant external details, visible only under high magnification, are not mentioned)  
Natural not shown.

CLARITY GRADE (10 x) : INTERNALLY FLAWLESS

COLOR GRADE : G.(1)

FLUORESCENCE : NONE

Control Department

LABORATORY DIRECTOR, GEMMOLOGIST

#### SPACE FOR DOUBLE-CHECK, CLARITY- AND COLOR GRADE

CLARITY GRADE:	Flawless, internally FL	vvs 1	vvs 2	vs 1	vs 2	si 1	si 2	p 1	p 2	p 3							
COLOR GRADE:	0+ D	0 E	1+ F	1 G	2 H	3 I	4 J	5 K	6 L	7 M	8 N	9 O	10 P	11 Q	12 R	13 20	FANCY COLOR

PROPORTIONS - MARGIN : ± 1%

\* MEASUREMENTS - MARGIN : ± 0,03 mm.

This report is subject to the terms and conditions set forth on the reverse.